

Front panel and display

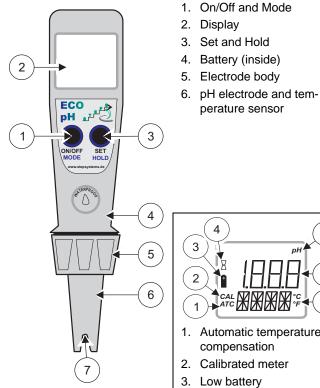



- compensation
- 2. Calibrated meter
- 3. Low battery
- 4. Stability indicator
- 5. Measurement unit
- 6. Measurement display
- 7. Temperature display

Technical data

Range	0 to 14 pH, -5 to 60°C (23 to 140°F)
Resolution	0,01 pH, 0,1°C (0,1°F)
Accuracy	± 0,01 pH, ± 0,5°C (± 1°F)
Calibration	automatic 1- or 2-point calibration
Temperature com- pensation	automatic
Battery	4 x 1,5V button type, approx. 100 hours of use
Auto-off	after 8 minutes of non-use
Envirment	-5 to 50°C (23 to 122°F), RH 100%
Housing	waterproof
Dimension	175,5 x 39 x 23 mm
Weight	100 g
Warranty	1 year, 3 month electrode

Operation

Turn on and measurement

- 1. Press and hold **ON/OFF** until the display lights up.
- 2. Remove the protective cap of the electrode. The tester is now ready for operation.
- 3. Put the electrode into the sample. The stability indicator shows a stable measurement result.
- 4. Freeze the display with SET/HOLD. Press any button to return to measurement mode.
- 5. To turn off the tester press ON/OFF until the display shows OFF.
- 6. Clean the electrode after each measurement session with distilled water. Put a few drops calibration solution pH 4,01 in the protective cap and put on the cap.

Do **never** store the electrode in destilled water.

Calibration

Calibrate the ECO pH-Tester, if

- the electrode has been replaced ٠
- ٠ min. once per week
- ٠ to ensure accurate results
- after measuring agressive chemicals
- Press and hold ON/OFF, until the display shows CAL. 1.
- Release ON/OFF, the display shows pH 7.01 USE. 2.
- Put the electrode in the calibration solution pH 7.01. The CAL-3. symbol flashes, until the display shows pH 4.01 USE.
- To finish the 1-point calibration, press ON/OFF, the tester 4 shows OK 1 and returns to the measurement mode.
- For a 2-point-calibration, clean the electrode and put it in the 5. calibration solution pH 4.01. The CAL-symbol flashes.
- The display shows **OK 2**, when the calibration is successful. 6. The tester returns to the measurement mode.

Maintenance

Change the electrode

- 1. Unscrew the retaining ring and put it off.
- 2. Pull off the old electrode body.
- 3. Put on the new electrode body.
- 4. Screw the retaining ring on.
- 5. Calibrate the electrode.

Change the battery

- 1. When the display shows the battery icon, change the batteries.
- 2. Unscrew the retaining ring and put it off.
- 3. Pull off the electrode body.
- 4. Pull out the battery compartment gently.
- 5. Change the four 1,5V button batteries, pay attention to the polarity.
- 6. Press the battery compartment carefully back into the ECO pH-Tester.
- 7. Put on the electrode body.
- 8. Screw the retaining ring on.
- 9. Calibrate the electrode.



STEP Systems GmbH

Duisburger Str. 44 D-90451 Nürnberg Tel: 0049 (0) 911-96 26 050 Fax: 0049 (0) 911-96 26 059 e-Mail: info@stepsystems.de Internet: www.stepsystems.de Printed in Germany 2016 All rights reserved